

Dialyzer

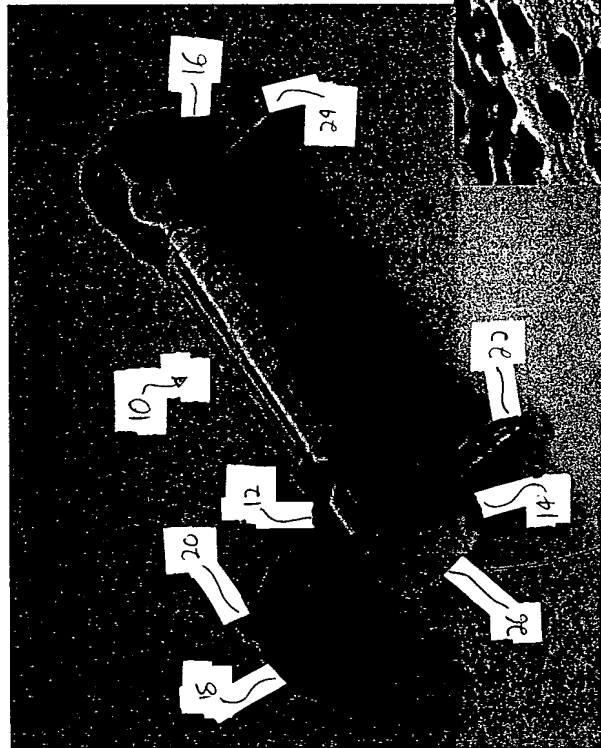


Fig. 1

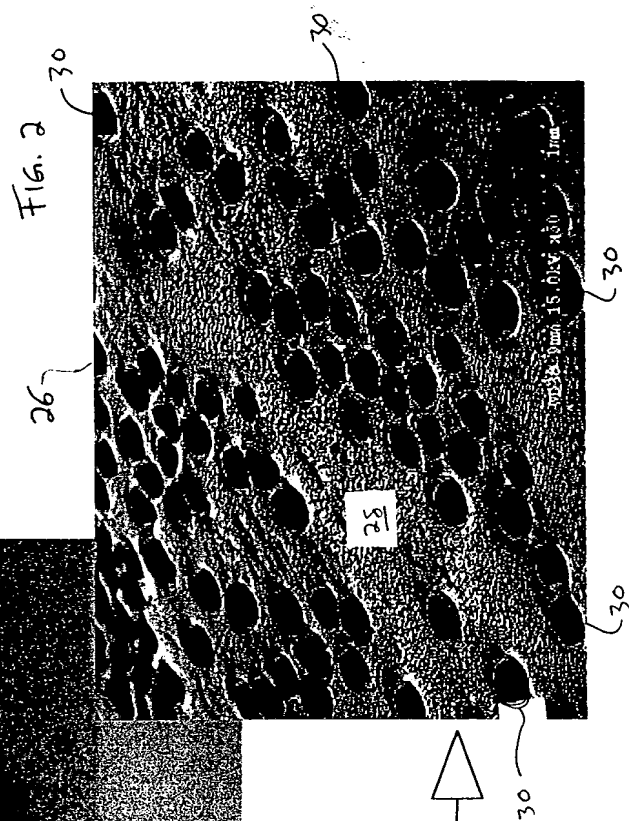


Fig. 2

Dialyzer fiber morphology.

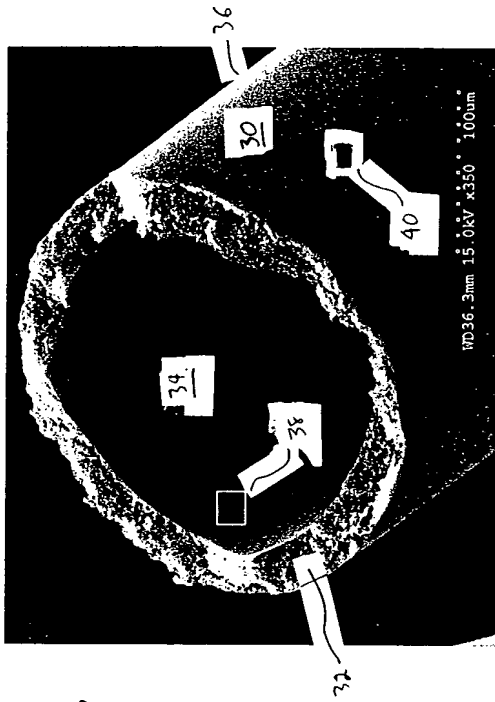


FIG. 3

FIG. 4


Fiber interior surface.



34

FIG. 5

Fiber exterior surface.

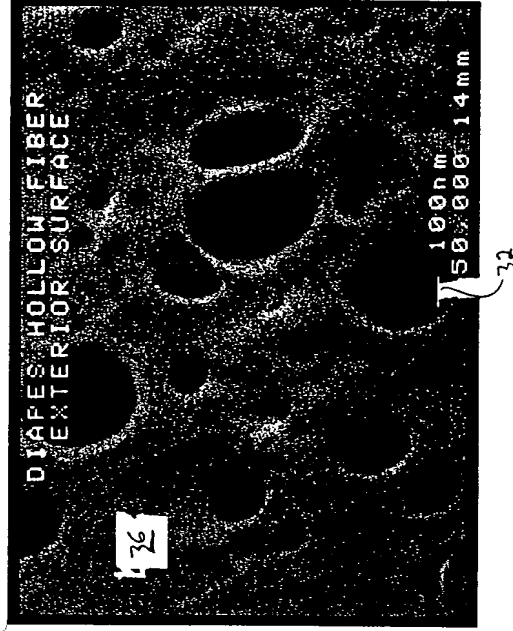

36

Fig. 6
DRY TEST FLOWPATH DIAGRAM

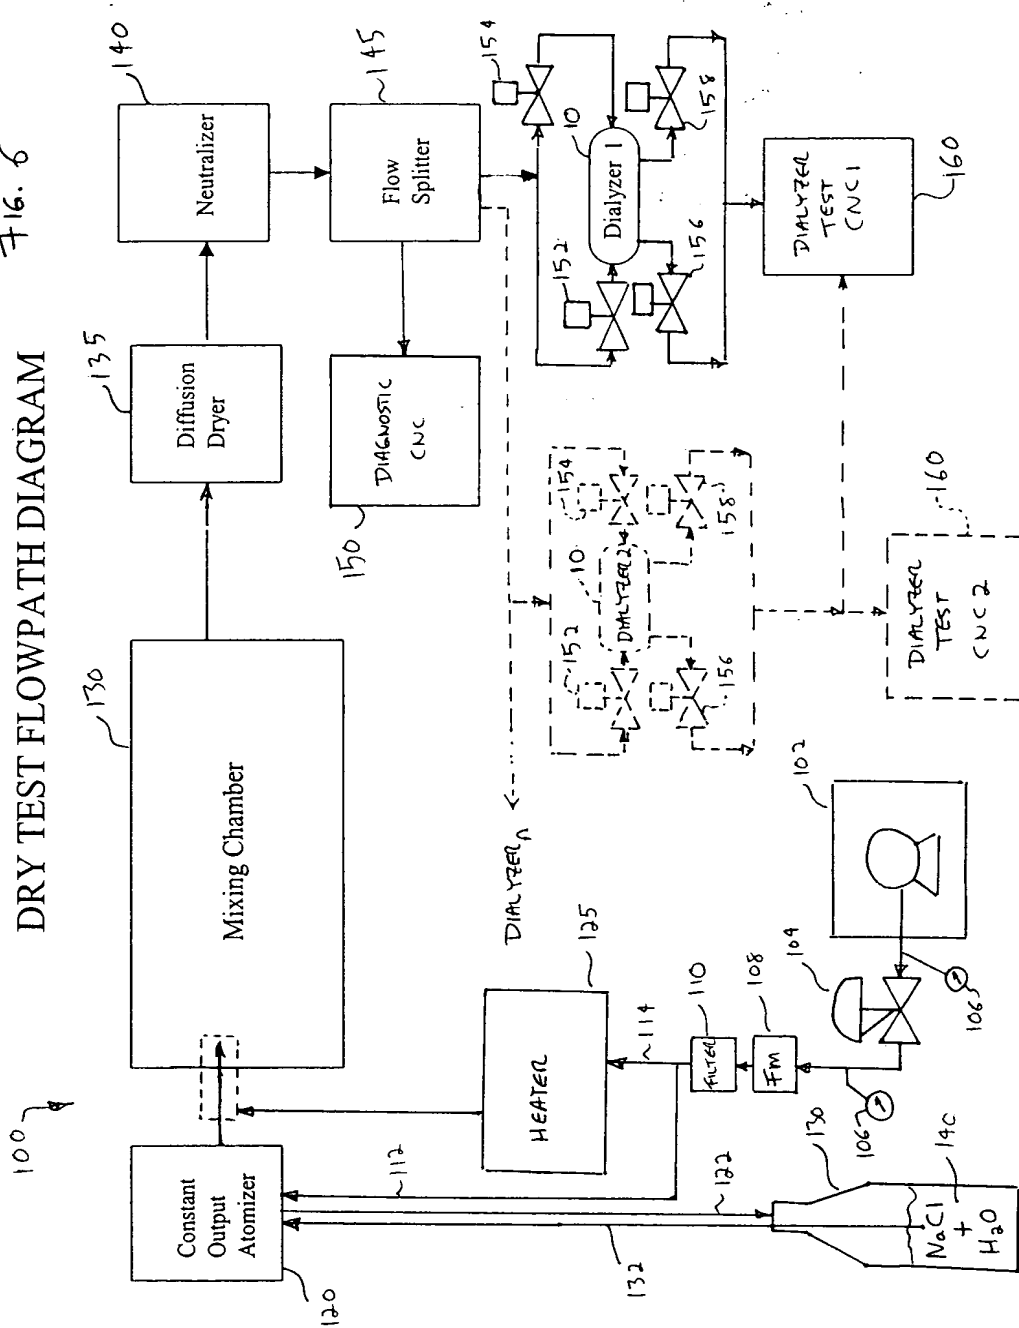


FIG. 7

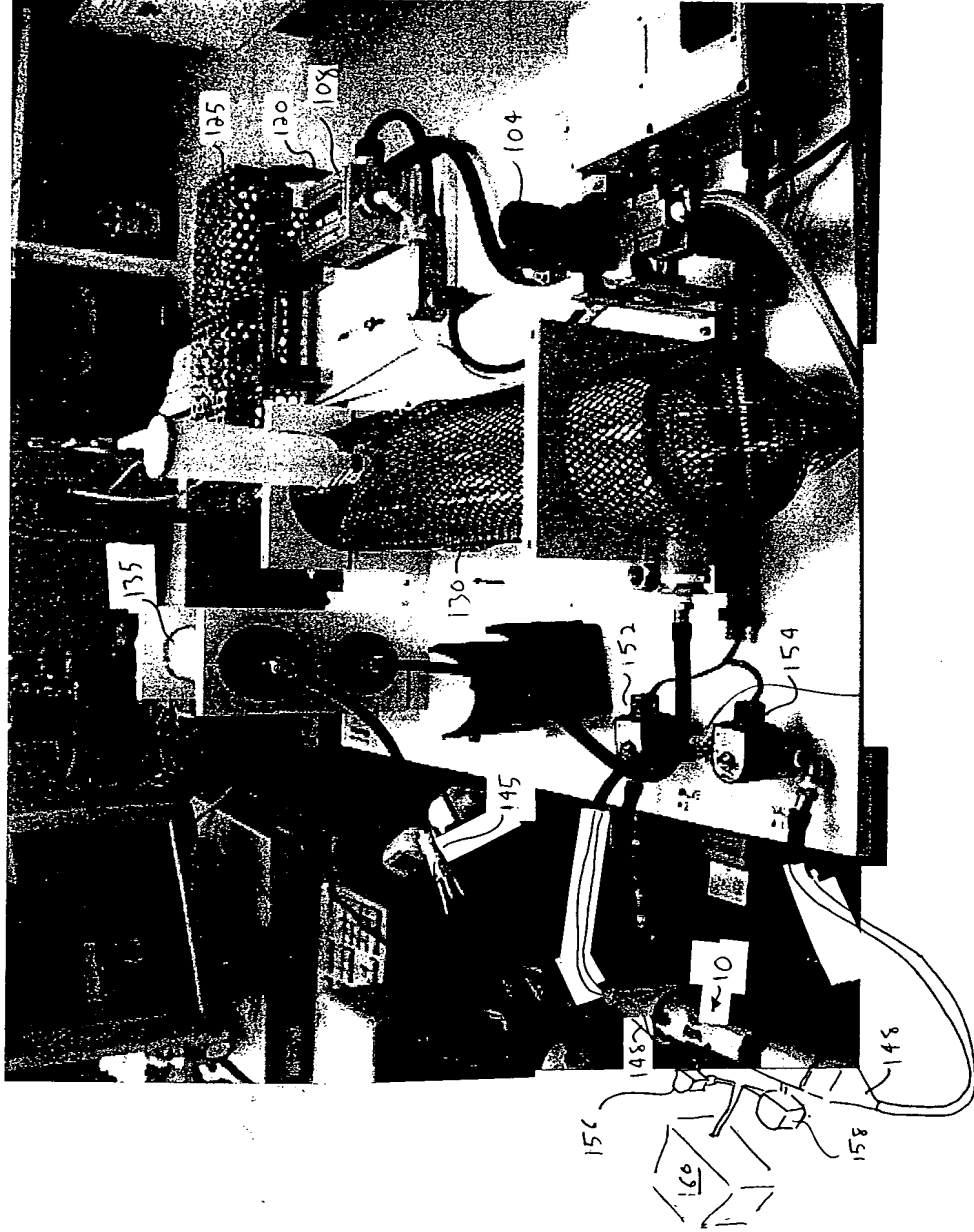


FIG. 8

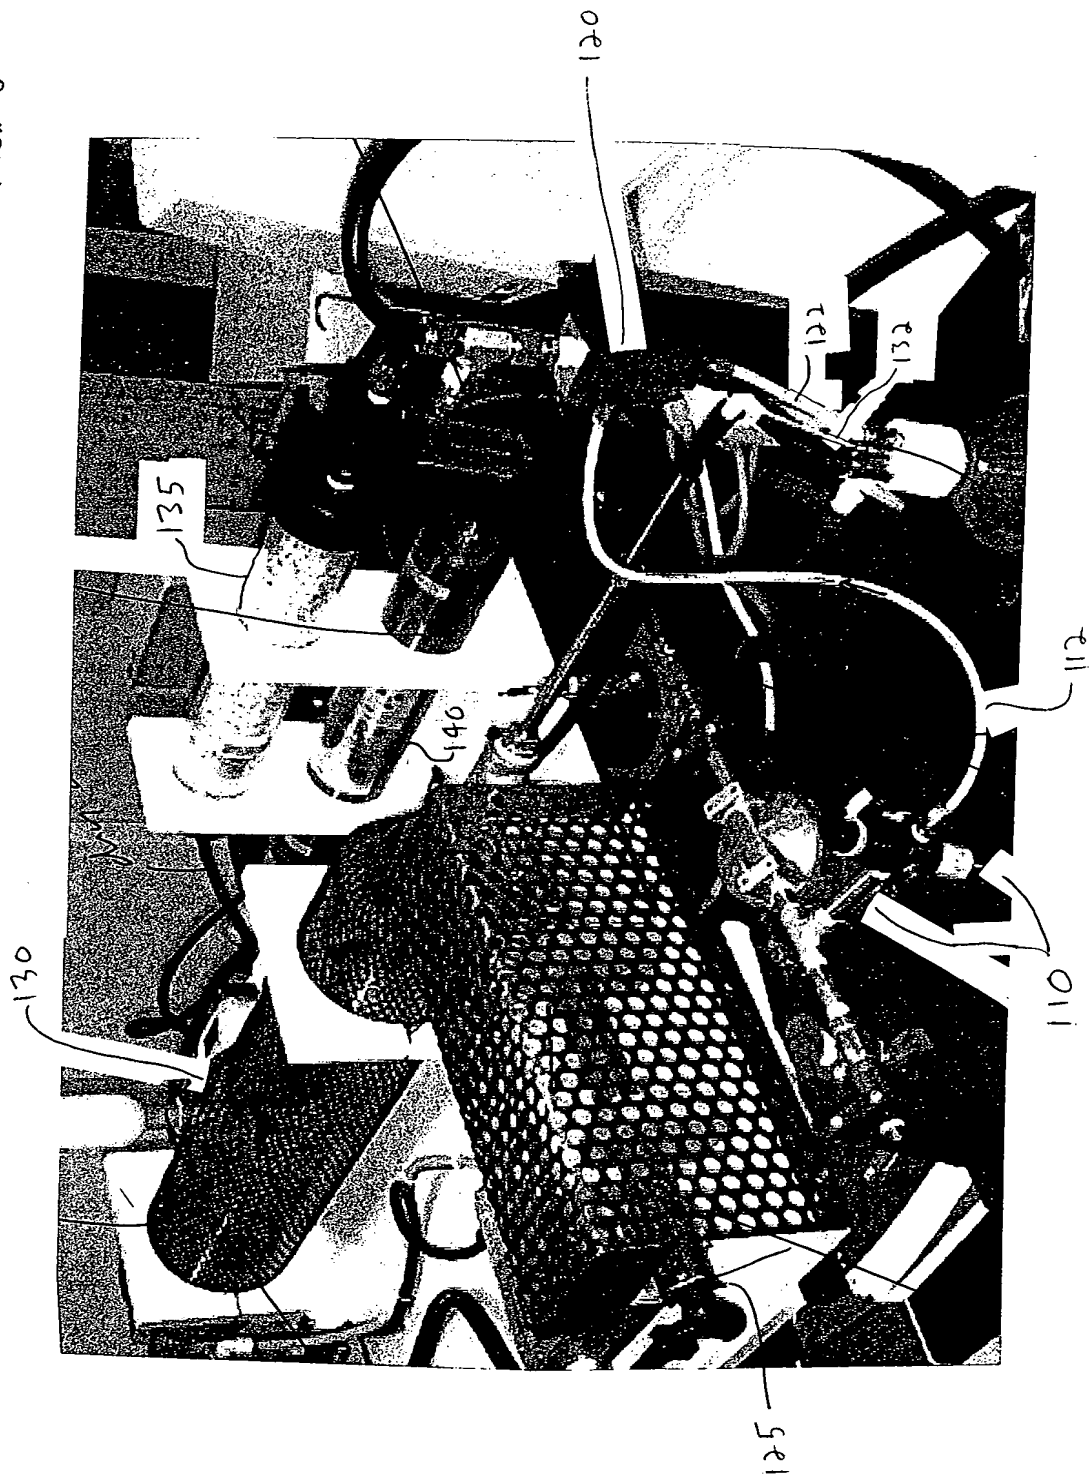


FIG. 9A

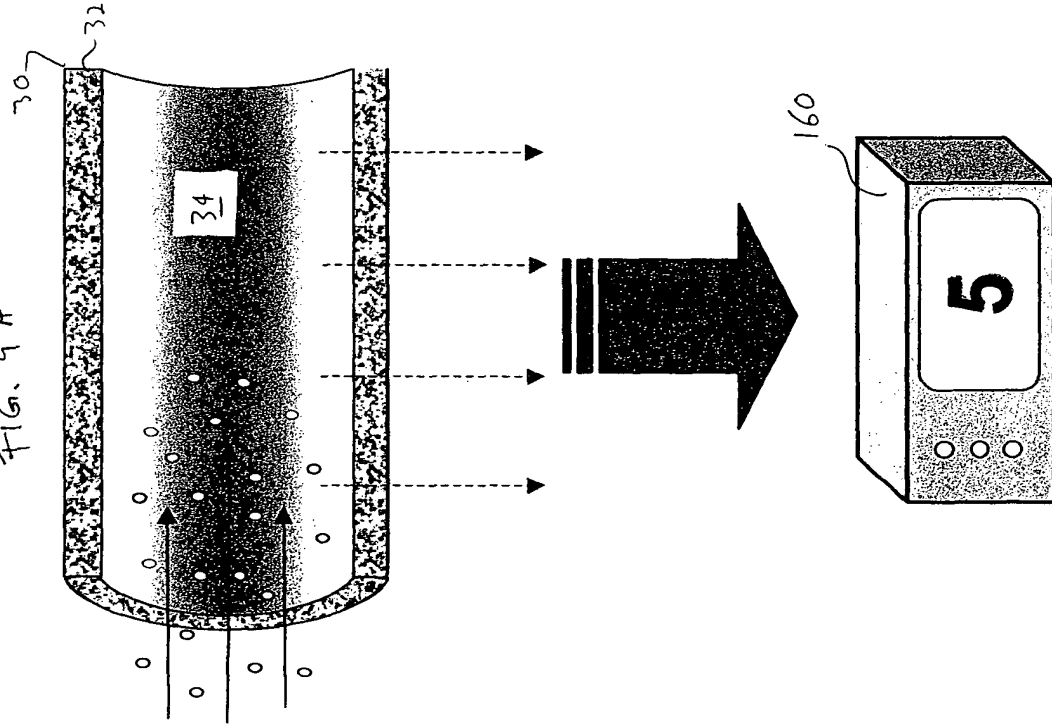


FIG. 9B

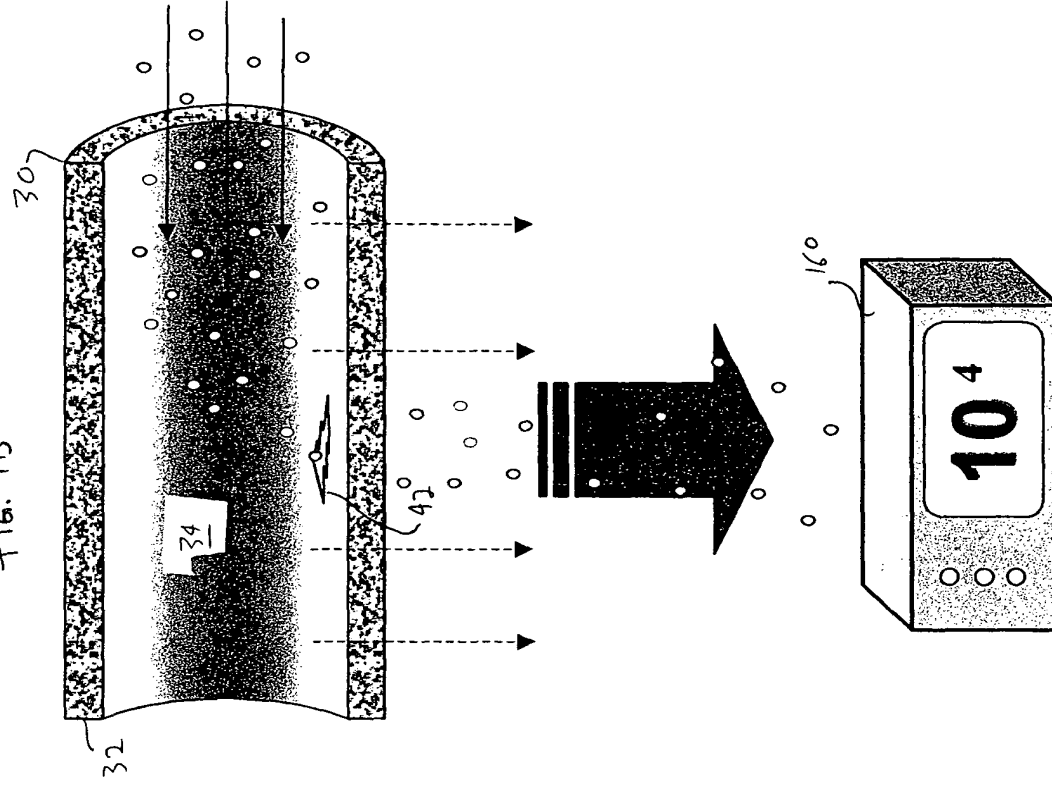




FIG. 10

